


TauroPace™




Generator substitution or revision

STEP BY STEP
INSTRUCTIONS

PREPARATION:


1

Surgical skin preparation must be carried out as close as possible to commencement of the procedure with an antiseptic solution recommended (consider fascial plane block for local anesthesia).

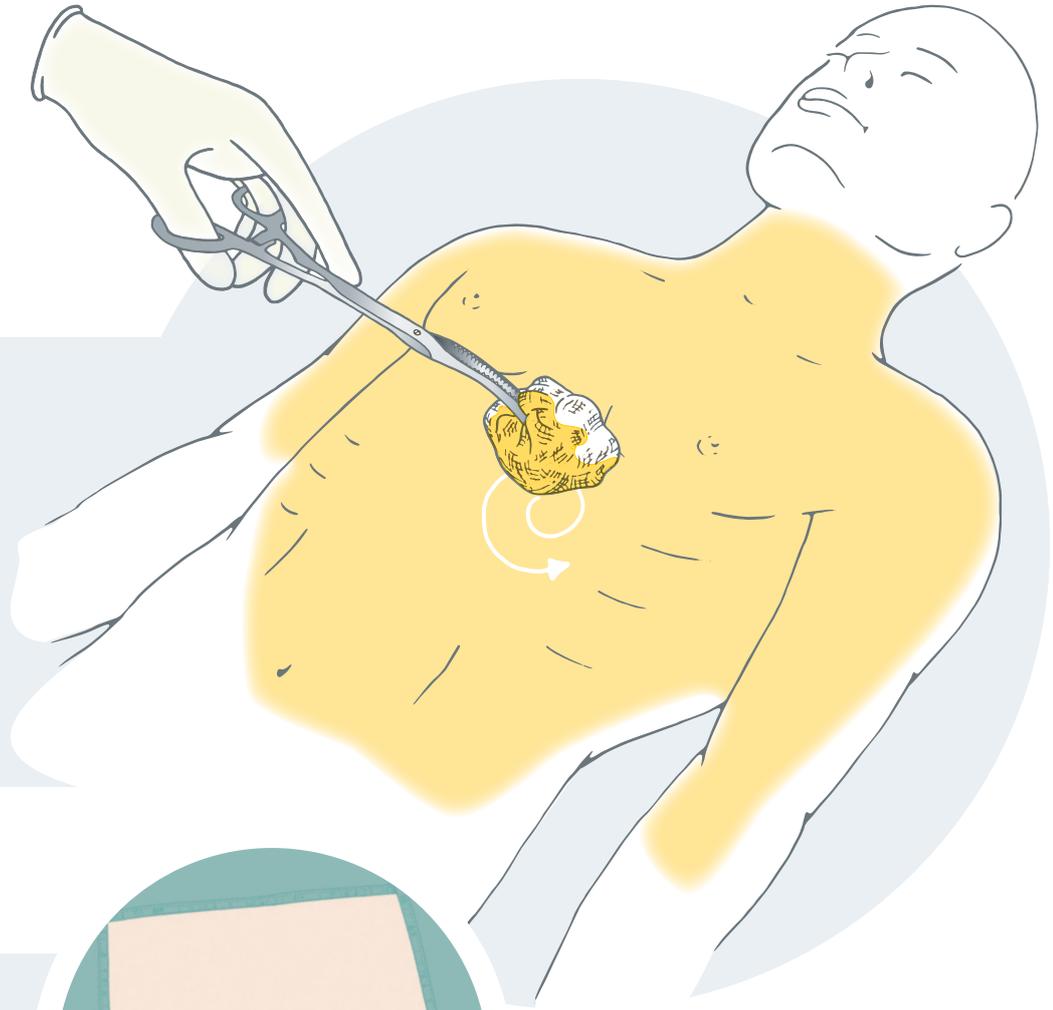


2

Drape the patient.


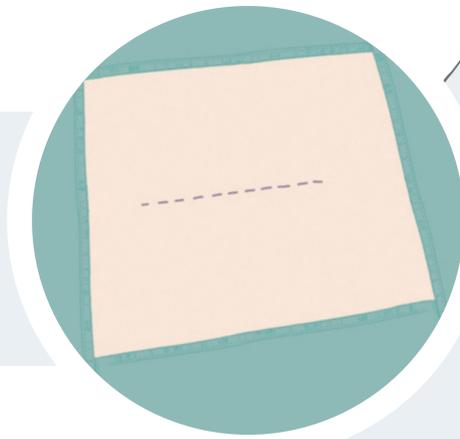


3


Transfer **TauroPace™** to a gallipot containing surgical swabs.

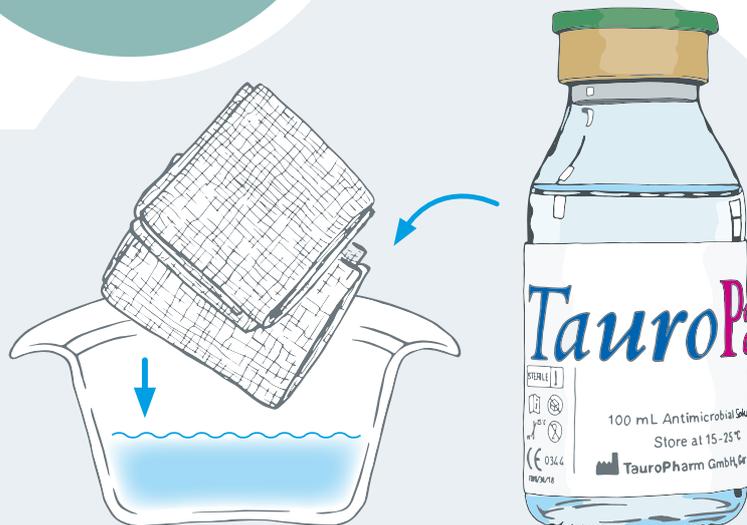


 **TauroPace™**
 antiseptic solution

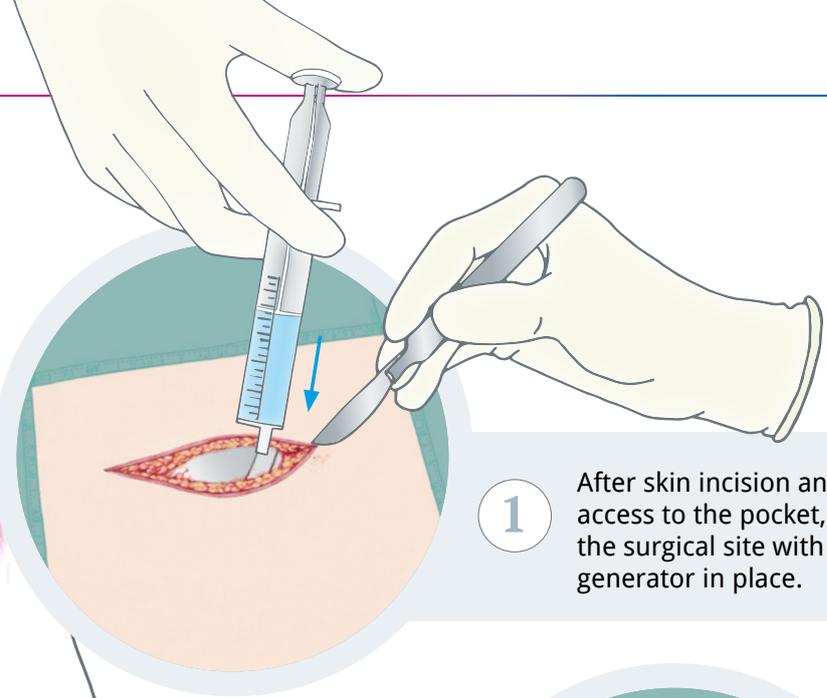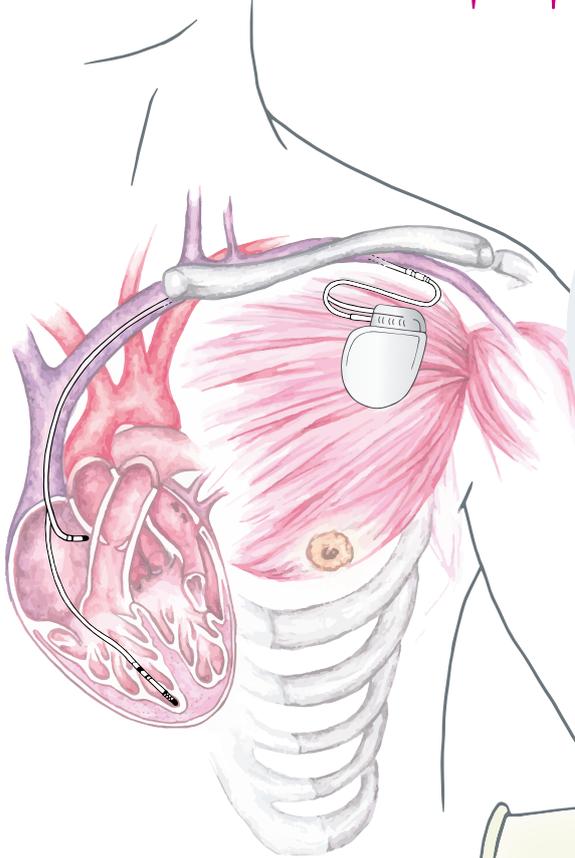



1 After skin incision and gaining access to the pocket, rinse the surgical site with the old generator in place.

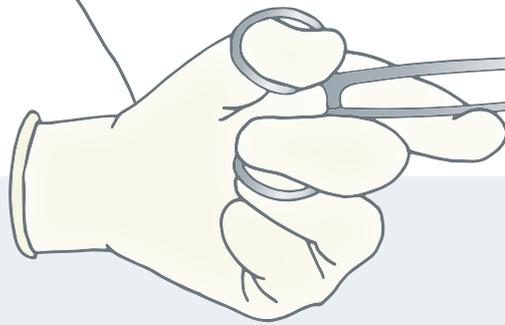


2 Mobilise the old generator.

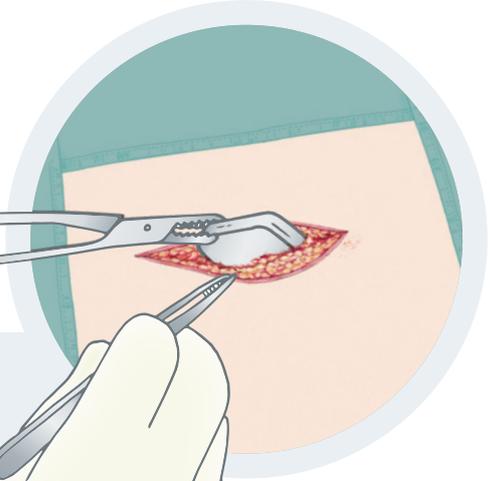


3 Immerse the torque wrench in TauroPace™.

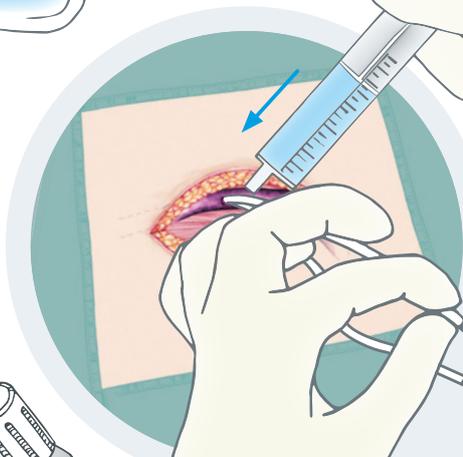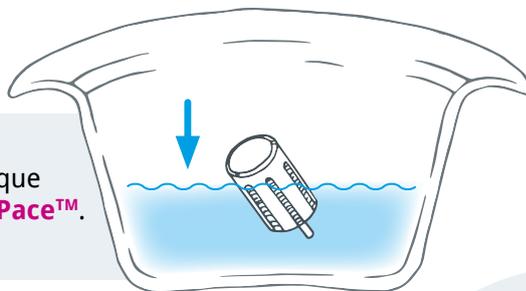

5 Disconnect the old generator, wipe the old leads down with a TauroPace™ soaked swab and rinse the surgical site with TauroPace™.

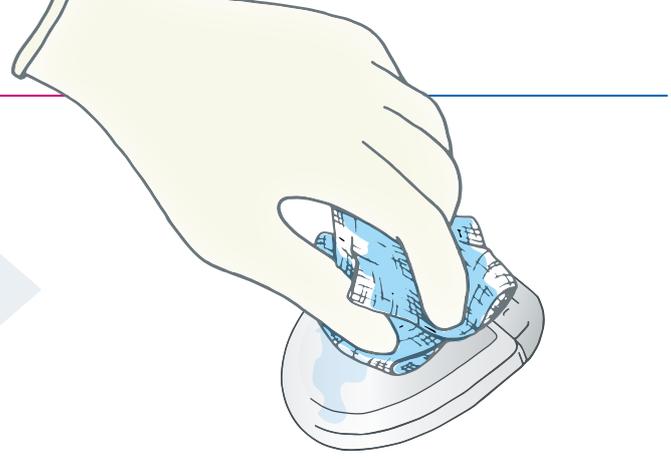


6 Wipe the new generator down with a **TauroPace™** soaked swab.

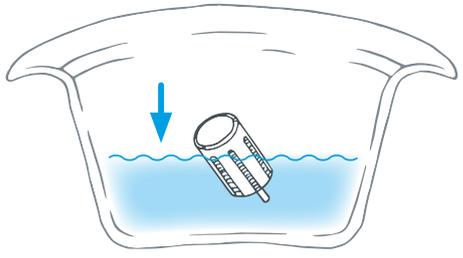


7 Immerse the torque wrench in **TauroPace™**.

8 Connect the lead(s) to the generator; use **TauroPace™** soaked swabs to hold on to the lead and the generator.

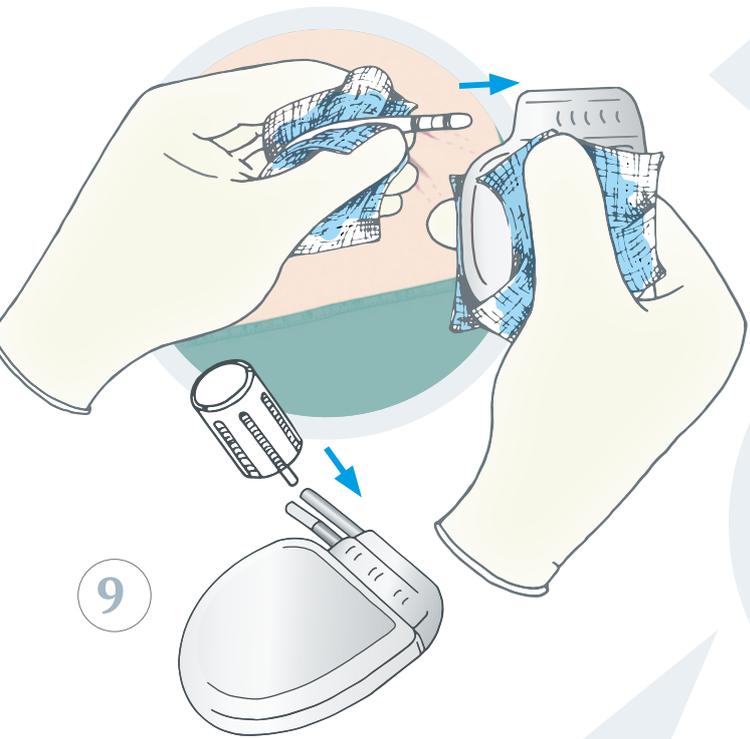


9

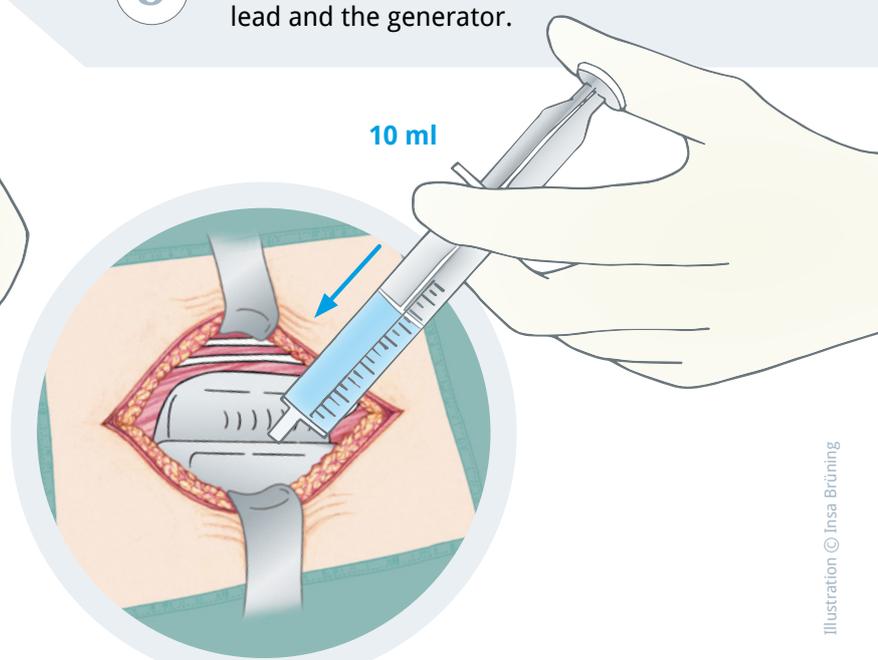

10 After final placement of all hardware, rinse the surgical site with **TauroPace™**.

11 Remove excess **TauroPace™**.

AFTER SKIN CLOSURE:

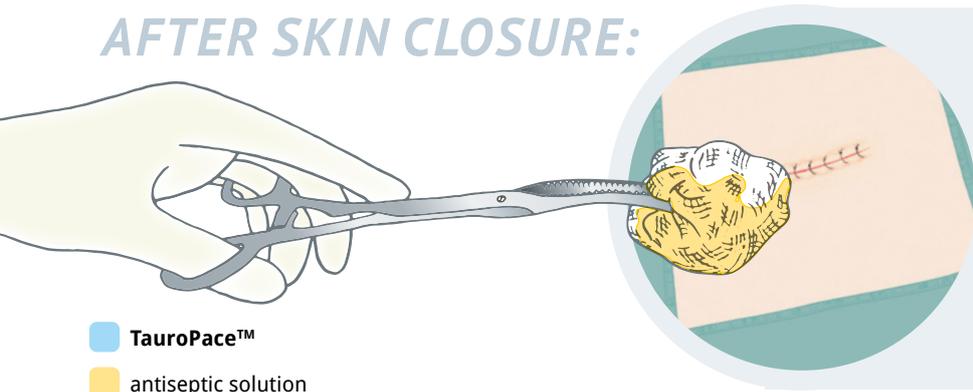

- 1 After skin closure wipe down with recommended skin antiseptic.
- 2 Apply a sterile wound dressing.

Use one bottle of **TauroPace™** per procedure.

TauroPace™
 antiseptic solution